

HOBOnet® Wireless Sensor Network

RXW Temperature/RH Sensor (RXW-THC-B-xxx) Manual



RXW Temperature/ RH Sensor

Models:

- RXW-THC-B-900 (US)
- RXW-THC-B-868 (Europe)
- RXW-THC-B-921 (Taiwan)
- RXW-THC-B-922 (Australia/NZ)

Included Items:

- Cable ties
- Screws

The RXW Temperature/RH sensor measures temperature and RH and is designed to work with the HOBOnet Wireless Sensor Network in which data is transmitted wirelessly from the sensor mote across the network to the station and then uploaded to HOBOLink. With HOBOLink, you can monitor sensor readings, view graphs, set up alarms, download data, and more.

Specifications

Sensor	Temperature	RH
Measurement Range	-40°C to 75°C (-40°F to 167°F)	0–100% RH at -40° to 75°C (-40° to 167°F); exposure to conditions below -20°C (-4°F) or above 95% RH may temporarily increase the maximum RH sensor error by an additional 1%.
Accuracy	±0.25°C from -40° to 0°C (±0.45°F from -40° to 32°F) ±0.20°C from 0° to 70°C (±0.36°F from 32° to 158°F) ±0.25°C from 70° to 75°C (±0.45°F from 158° to 167°F)	±2.5% from 10% to 90% RH typical to a maximum of ±3.5% including hysteresis at 25°C (77°F); below 10% and above 90% ±5% typical.
Resolution	0.02°C (0.036°F)	0.01% RH
Drift	<0.01°C (0.018°F) per year	<1% per year typical
Response Time (typical, to 90% of change)	3 minutes, 45 seconds in air moving 1 m/s	15 seconds in air moving 1 m/s
Wireless Mote		
Operating Temperature Range	-40° to 70°C (-40° to 158°F)	
Radio Power	12.6 mW (+11 dBm) non-adjustable	
Transmission Range	Reliable connection to 457.2 m (1,500 ft) line of sight at 1.8 m (6 ft) high Reliable connection to 609.6 m (2,000 ft) line of sight at 3 m (10 ft) high	
Wireless Data Standard	IEEE 802.15.4	
Radio Operating Frequencies	RXW-THC-B-900: 904–924 MHz RXW-THC-B-868: 866.5 MHz RXW-THC-B-921: 921 MHz RXW-THC-B-922: 916–924 MHz	
Modulation Employed	OQPSK (Offset Quadrature Phase Shift Keying)	
Data Rate	Up to 250 kbps, non-adjustable	
Duty Cycle	<1%	
Maximum Number of Motes	Up to 50 wireless sensors or 336 data channels per one HOBOnet RX station	
Logging Rate	1 minute to 18 hours	
Number of Data Channels	3	
Battery Type	Two AA 1.5 V lithium batteries	
Battery Life	1 year, typical use	
Memory	16 MB	
Dimensions	Sensor: 45.97 x 11.43 x 10.16 mm (1.81 x 0.45 x 0.40 inches) Mote: 16.2 x 8.59 x 4.14 cm (6.38 x 3.38 x 1.63 inches)	
Weight	223 g (7.87 oz)	
Materials	Sensor: Polyamide Mote: PCPBT, silicone rubber seal	
Environmental Rating	IP67, NEMA 6	

Specifications (continued)

Compliance Marks



RXW-THC-B-900: See the last page.



RXW-THC-B-868: The CE Marking identifies this product as complying with all relevant directives in the European Union (EU).




RXW-THC-B-921: See the last page.



RXW-THC-B-922: See the last page.

Mote Components and Operation

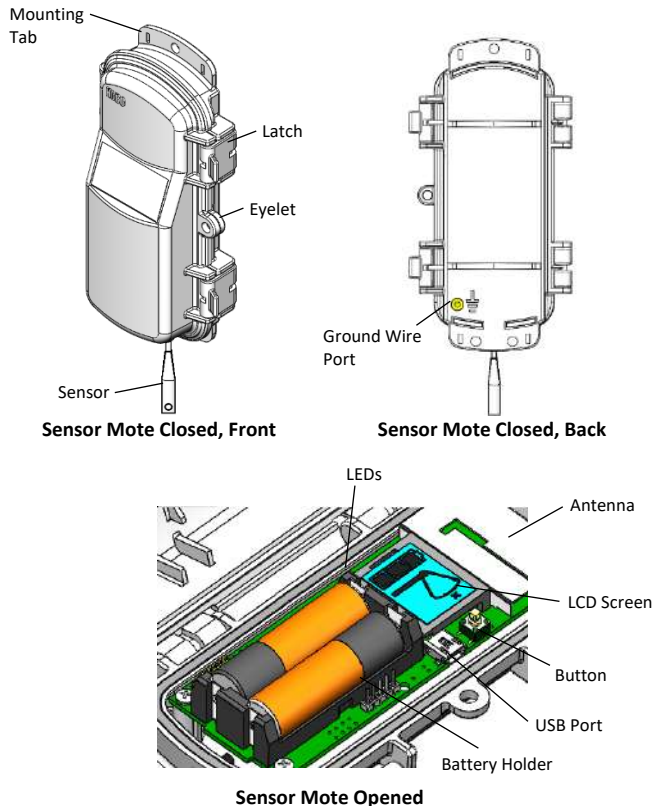

Mounting Tab: Use the tabs at the top and bottom of the mote to mount it (see [Deploying and Mounting](#)).

Sensor: This is the temperature/RH sensor connected to the mote.

Eyelet: Use this eyelet to attach a 3/16 inch padlock to the mote for security.

Latch: Use the two latches to open and close the mote door.

Ground Wire Port: Use this port to connect a ground wire (see [Deploying and Mounting](#)).

Antenna: This is the built-in antenna for the radio communications across the wireless network.

LEDs: There are two LEDs to the left of the LCD screen. The green LED blinks during the process of joining a network, blinking quickly while the mote searches for a network and then slowly as the mote registers with the network. Once the network registration process is complete, the blue LED blinks at 4 seconds to indicate normal operation. If the mote is not currently part of a network, the blue LED will be off. If the blue LED is on and not blinking, there is a problem with the mote. Contact Onset Technical Support.

Battery Holder: The location where the batteries are installed as shown (see [Battery Information](#)).

USB Port: Use this port to connect to the mote to a computer via USB cable if you need to update the firmware (see [Updating Mote Firmware](#)).

Button: Push this button for 1 second to illuminate the LCD or 3 seconds for the mote to search for a wireless sensor network to join (see [Adding the Mote to the HOBOnet Wireless Sensor Network](#)).

LCD Screen: The mote is equipped with an LCD screen that displays details about the current status. This example shows all symbols illuminated on the LCD screen followed by definitions of each symbol in the table.



LCD Symbol	Description
	The battery indicator shows the approximate battery charge remaining.
	The signal strength indicator shows signal strength bars. The more bars, the stronger the signal between motes. If there is no X icon next to the signal strength indicator, the mote is part of a HOBOnet Wireless Sensor Network.
	An empty signal strength indicator with the X icon indicates that the mote is not currently part of a network. See Adding the Mote to the HOBOnet Wireless Sensor Network for details on how to add a mote to the network.
	While the mote is joining a network, the signal strength indicator blinks and the bars in the icon cycle from left to right. The X icon blinks during the last step in the network registration process (see Adding the Mote to the HOBOnet Wireless Sensor Network for details).
	Indicates a problem with the sensor itself (the mote is operational). Check the sensor and make any adjustments to it as needed. Contact Onset Technical Support by calling 1-508-759-9500 or by clicking Onset Technical Support if the problem persists.


Adding the Mote to the HOBOnet Wireless Sensor Network

The mote must join a HOBOnet Wireless Sensor Network before it can begin measuring temperature and RH and transmitting data. This requires accessing the station and the mote at the same time so it is recommended that you complete these steps before deploying the mote.


Important: If you are setting up a new station, follow the instructions in the station quick start before setting up this mote: [HOBO MicroRX Station for HOBOnet \(RX2105 and RX2106\) Quick Start Guide](#) or [HOBO RX3000 Remote Monitoring Station Quick Start Guide](#).

To add a mote to the network:


1. If the LCD on the station is blank, press any button to wake it up.
2. Press the Select button once (which shows the number of smart sensors installed) and then press it again to switch to the module where the manager is installed (module 2 on RX2105 or RX2106 stations).

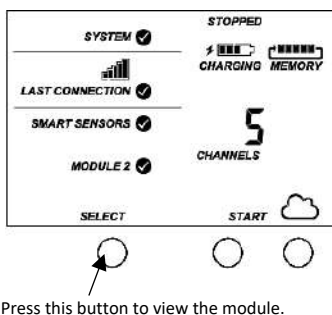

3. Press the Search button (the magnifying glass). The magnifying glass icon blinks while the station is in search mode.

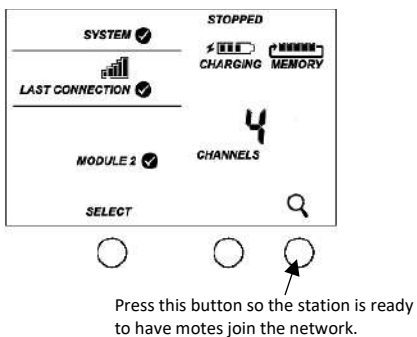


4. Open the mote door and install the batteries if you have not already done so.
5. Press the button on the mote for 3 seconds. The signal strength icon flashes and then cycles.

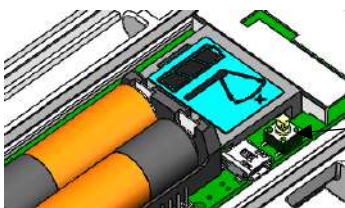

Press this button for 3 seconds for the mote to join the network.

6. Watch the LCD on the mote.



The signal strength icon blinks while the mote is searching for a network.



Once the mote finds a network, the icon stops flashing and the bars cycle from left to right.



The network connection X icon blinks while the mote completes the registration process, which may take up to five minutes.




Once the mote has finished joining the network, the X icon disappears and the channel count on the station LCD increases by three (two for temperature/RH and one for the mote battery).

This process may take up to five minutes. The green LED blinks quickly while the mote searches for a network to join and then blinks slowly while it completes the network registration. Once the mote has finished joining the network, the green LED turns off and the blue LED then blinks indefinitely while the mote is part of the network.

Note: If the mote cannot find the network or has trouble remaining connected during this process, make sure the mote is in a vertical, upright position and within range of the station.

7. Press the Search button (the magnifying glass) on the station to stop searching for motes.

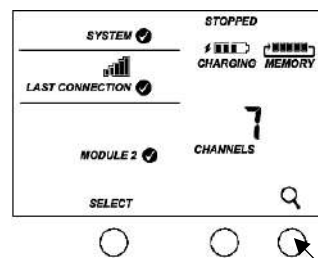

Press this button again to stop searching for motes.

If you added more than one more mote to the network, the total channel count for the module on the station LCD represents all measurement channels plus a battery channel for each mote in the network.

Sensor measurements are recorded at the Logging Interval specified in HOBOLink, transmitted to the station, and uploaded to HOBOLink at the next connection interval. Use HOBOLink to monitor mote status and health. If a mote is temporarily offline, any logged data is saved until it is back online. In addition, if a mote is offline for 30 minutes, the station automatically connects to HOBOLink and reports the mote as missing. Once the mote is back online, any logged data is uploaded the next time the station connects to HOBOLink.

See the [HOBOLink Online Help](#) for details on how to change the logging and connection intervals, view data, check mote status, add the mote to a map, and more.

Deploying and Mounting

Mounting and Positioning the Mote

- Mount the mote on a mast or pipe using cable ties or affix the mote to a wooden post or flat surface with screws. Insert the cable ties or screws through the holes on the mounting tabs.
- Consider using plastic poles such as PVC to mount the mote since certain types of metal could decrease signal strength.
- Make sure the mote remains in a vertical position once it is placed in its deployment location for optimal network communications.
- Make sure the mote door is closed, with both latches fully locked to ensure a tight seal.
- Consider using a 3/16 inch padlock to restrict access to the mote. With the mote door closed, hook a padlock through the eyelet on the right side of the door and lock it.
- Make sure the mote is mounted a minimum of 1.8 m (6 ft) from the ground to help maximize distance and signal strength.
- Place the mote so there is full line of sight with the next mote. If there is an obstruction between two sensor motes or between the sensor mote and the manager, use a repeater mounted on the obstruction.
- There should not be more than five motes in any direction at their maximum transmission range from the manager. Data logged by a wireless sensor must travel or “hop” across the wireless network from one mote to the next until it ultimately reaches the manager connected to the station. To make sure data can successfully travel across the network, the mote should not be more than five hops away from the manager.
- The HOBOnet Wireless Sensor Network can support up to 50 wireless sensors or 336 data channels per one HOBOnet RX station.
- Use a #4-40 screw to attach a ground wire to the port on the back of the mote if you are deploying the mote in a location where lightning is a concern.

Sensor Mounting Guidelines

- We recommend that you protect the probe direct exposure to the weather. This prolongs the sensor accuracy.
- See the [HOBOnet MicroRX Station for HOBOnet \(RX2105 and RX2106\) Manual](#) or the [HOBOnet RX3000 Remote Monitoring Station User's Manual](#) and [Tripod Setup Guide](#) for more information regarding setting up stations.

Maintenance

The temperature/RH sensor is sensitive to dust, salts, and other airborne contamination. Periodically inspect the RH sensor. If contamination is present on the protective cap, gently rinse it with cool fresh water. If the sensor itself is contaminated, you can rinse it with distilled water. Do not use hot water, organic solvents, or detergents. Dry before use.

Periodically inspect the mote and do the following:

- Verify the mote is free of visible damage or cracks.
- Make sure the mote is clean. Wipe off any dust or grime with a damp cloth.
- Wipe off any water before opening the mote.
- Make sure the interior seal is intact and the latches are fully locked when the mote door is closed.

Updating Mote Firmware

If you have trouble with your mote, contact Onset Technical Support by calling 1-508-759-9500 or by clicking here: [Onset Technical Support](#) who will provide an update file, if you need one. To install that file:

1. Connect the mote to the computer with a USB cable (open the mote door and use the USB port to the right of the LCD). The blue LED is illuminated while connected.
2. The mote appears as a new storage device in the computer's file storage manager. Copy the downloaded firmware file to the new storage device (the mote). The blue LED blinks slowly while the file is copying.
3. After the file is copied to the mote, the LED stops blinking and remains a steady blue. Eject the storage device from the computer and disconnect the cable from the mote. The firmware installation process begins automatically on the mote. The blue LED blinks rapidly while the firmware is installed. Once the firmware installation is complete, the LCD symbols return and the mote automatically rejoins the network.

Notes:

- Mac® users: A message may appear indicating the disk has not ejected properly when disconnecting the mote from the computer. The mote is operational and you can ignore the message.
- If the blue LED turns off abruptly while copying the file or installing the firmware, a problem has occurred. Contact Onset Technical Support by calling 1-508-759-9500 or by clicking here: [Onset Technical Support](#).

Battery Information

The mote uses two 1.5 V lithium batteries (HWSB-LI). Lithium battery life is estimated at 1 year, but varies based on the ambient temperature where the mote is deployed, the logging interval, the number of tripped alarms, and other factors. Estimates are not guaranteed due to uncertainties in initial battery conditions and operating environment.

To install lithium batteries:

1. Open the mote door.
2. Remove any old batteries and install the new ones observing polarity.

The mote contacts the network once the new batteries are installed. The green LED blinks quickly while the mote searches for a network to join and then blinks slowly while it completes the network registration. Once the mote has finished joining the network, the green LED turns off and the blue LED then blinks indefinitely while the mote is part of the network.

⚠ WARNING: Do not cut open, incinerate, heat above 85°C (185°F), or recharge the lithium batteries. The batteries may explode if the mote is exposed to extreme heat or conditions that could damage or destroy the battery cases. Do not mix battery types, either by chemistry or age; batteries may rupture or explode. Do not dispose of the logger or batteries in fire. Do not expose the contents of the batteries to water. Dispose of the batteries according to local regulations for lithium batteries.

Federal Communication Commission Interference Statement

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one of the following measures:

- Reorient or relocate the receiving antenna
- Increase the separation between the equipment and receiver
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected
- Consult the dealer or an experienced radio/TV technician for help

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

FCC Caution: Any changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate this equipment.

Industry Canada Statements

This device complies with Industry Canada license-exempt RSS standard(s). Operation is subject to the following two conditions: (1) this device may not cause interference, and (2) this device must accept any interference, including interference that may cause undesired operation of the device.

Avis de conformité pour l'Industrie Canada

Le présent appareil est conforme aux CNR d'Industrie Canada applicables aux appareils radio exempts de licence. L'exploitation est autorisée aux deux conditions suivantes : (1) l'appareil ne doit pas produire de brouillage, et (2) l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

To comply with FCC and Industry Canada RF radiation exposure limits for general population, the logger must be installed to provide a separation distance of at least 20cm from all persons and must not be co-located or operating in conjunction with any other antenna or transmitter.

NCC Statement

經型式認證合格之低功率射頻電機，非經許可，公司、商號或使用者均不得擅自變更頻率、加大功率或變更原設計之特性及功能。

低功率射頻電機之使用不得影響飛航安全及干擾合法通信；經發現有干擾現象時，應立即停用，並改善至無干擾時方得繼續使用。前項合法通信，指依電信法規定作業之無線電通信。低功率射頻電機須忍受合法通信或工業、科學及醫療用電波輻射性電機設備之干擾。

Translation:

Article 12

Without permission granted by the NCC, any company, enterprise, or user is not allowed to change frequency, enhance transmitting power or alter original characteristic as well as performance to an approved low power radio-frequency device.

Article 14

The low power radio-frequency devices shall not influence aircraft security and interfere with legal communications. If found, the user shall cease operating immediately until no interference is achieved. The said legal communications means radio communications is operated in compliance with the Telecommunications Act. The low power radio-frequency devices must be susceptible with the interference from legal communications or ISM radio wave radiated devices.